




# CERTIFICATE OF CALIBRATION AND TESTING

CUSTOMER: UNIVERSITY OF HAWAII  
P.O. NUMBER: Z10037157  
MODEL: 85106  
SERIAL NUMBER: UB02575

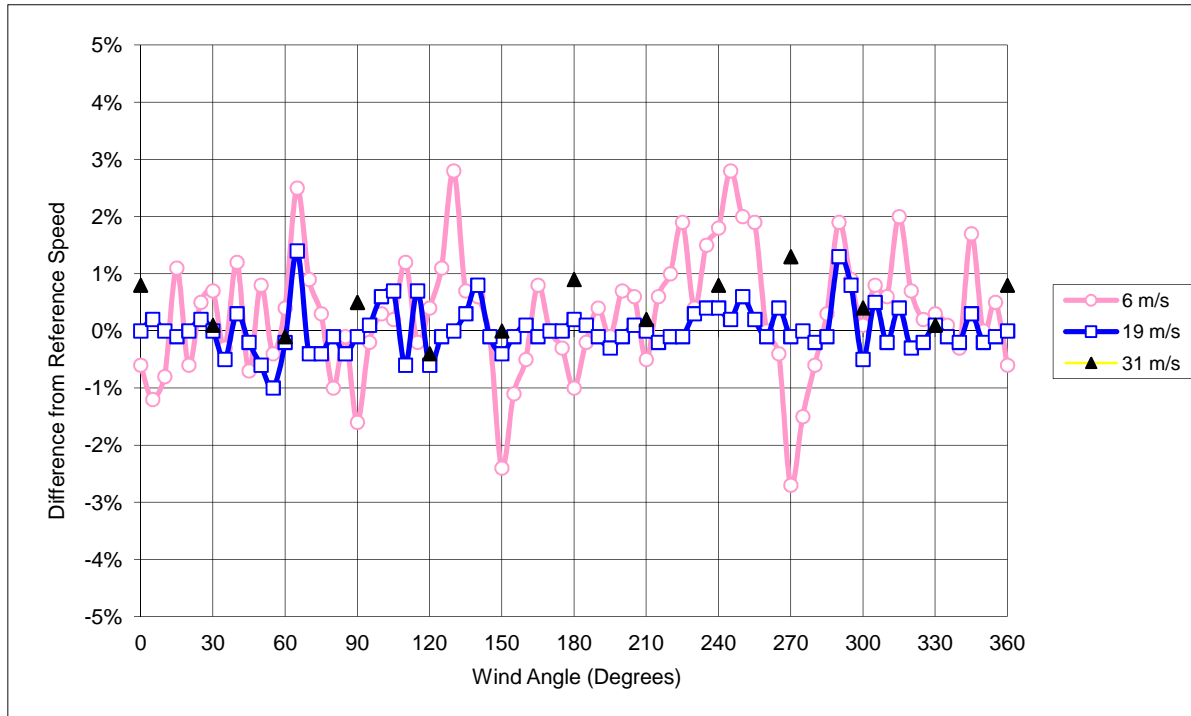

Speed (m/s)	Avg Diff	Std Dev
6.08	0.3%	1.1%
19.08	0.0%	0.4%
31.48	0.4%	0.5%

R. M. Young Company certifies that the above equipment was inspected and calibrated prior to shipment in accordance with established manufacturing and testing procedures. Standards established by R.M. Young Company for calibrating the measuring and test equipment used in controlling product quality are traceable to the National Institute of Standards and Technology.

To maintain these specifications, regular maintenance intervals are essential.

Calibration Date: 01 July 2013

R.M. Young Company

Ryan Phillips