

Chlorophyll WETStar Characterization

Date: March 19, 2013

S/N: WS3S-1352

Chlorophyll concentration expressed in $\mu\text{g/l}$ can be derived using the equation:

$$\text{CHL}(\mu\text{g/l}) = \text{Scale Factor} \times (\text{Output} - \text{Clean Water Offset})$$

	Analog output	Digital output
Clean Water Offset (CWO)	0.086 V @	87 counts
Scale Factor (SF)	5.4 $\mu\text{g/l/V}$ @	0.0065 $\mu\text{g/l/count}$
Maximum Output	5.48 V @	4095 counts
Resolution	0.69 mV	1 counts
Ambient Characterization Temperature	22 \pm 1 $^{\circ}\text{C}$	
Current Draw	60 mA @ 12V (typical)	
12-hour Stability	0.49 mV/hr	1 counts/hr
Temperature Stability, 25–2 $^{\circ}\text{C}$	0.21 mV/ $^{\circ}\text{C}$	1 counts/ $^{\circ}\text{C}$

Range	
15 $\mu\text{g/l}$	0
29 $\mu\text{g/l}$	X
150 $\mu\text{g/l}$	0

Definitions:

CWO: Clean Water Offset value obtained using pure filtered de-ionized water.

SF: Scale Factor is used to convert the fluorescence response of the instrument into chlorophyll-a concentration. Scale Factor is determined at WET Labs during a cross calibration using a liquid fluorescent standard and a reference fluorometer whose chlorophyll fluorescence response has been characterized in a laboratory using a mono-species lab culture of *Thalassiosira weissflogii* phytoplankton.

Maximum Output: Maximum signal output of the fluorometer.

Resolution: Standard deviation of 1 minute of clean water data, sampled once per second.


Ambient Characterization Temperature: Room temperature at time of characterization.

Current Draw: The amount of current the instrument uses for operation.

12-hour Stability: Deviation of output averaged over 12 hours.

Temperature Stability: Measured output variation per degree.

PO Box 518
620 Applegate St.
Philomath, OR 97370

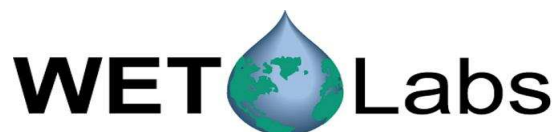

(541) 929-5650
Fax (541) 929-5277
www.wetlabs.com

WETStar Calibration and Repairs

Date March 19, 2013 **Customer** University of Hawaii Marine Center

S/N# WS3S-1352 **Repair Order** 18863

Standard Service

- Performed noise test: 1 sample/sec for 60 sec
- Performed stability test: 1 sample/min for 12 hrs
- Performed temperature test: 25–2 °C
- Performed saturation test
- Shake-tested unit
- Pressure-tested unit
- Updated unit's calibration sheet

Additional Repairs

Parts Replaced: Replaced Bulkhead Connector and O-Rings.

Comments

WETStar was re-calibrated with 25ppb Uranine.
Installed new 6 Pin Bulkhead Connector.
Digital / Analog Patch Cable Part #: EXA-210310