

APPLIED MICROSYSTEMS

003335 Certificate of Calibration

Customer: University of Hawaii
Asset Serial Number: 003335
Asset Type: 003335 SV Plus
Calibrated Pressure Range: 5000 dBar

Certification Date: 23/09/2009 (dd/mm/yyyy)

Certified By:


Applied Microsystems Ltd.

Robert Haydock,
President
Applied Microsystems

Applied Microsystems certifies that the equipment described above has been calibrated with equipment referenced to traceable standards. Any repairs / calibrations completed on this instrument were approved by the instrument owner under purchase order.


This instrument has been recalibrated. Please be sure to update your records. Please also ensure that you update the instrument's coefficient values in any post-processing software (ie. Smart Talk) that you use. Instrument configuration files are available at our Client Service & Support Portal (see web address below).

For a complete service history of this instrument, please consult our on-line Client Service & Support Portal at <http://www.appliedmicrosystems.com/customers/index.htm>

Applied Microsystems
2071 Malaview Avenue
Sidney, B.C. V8L 5X6 CANADA
Tel: +1-250-656-0771 Fax: +1-250-655-3655

Pressure Calibration

Date 09/23/09
S/N 003335
Calibrator Les Woodland
RMS 1.034
Range 5000 dBar

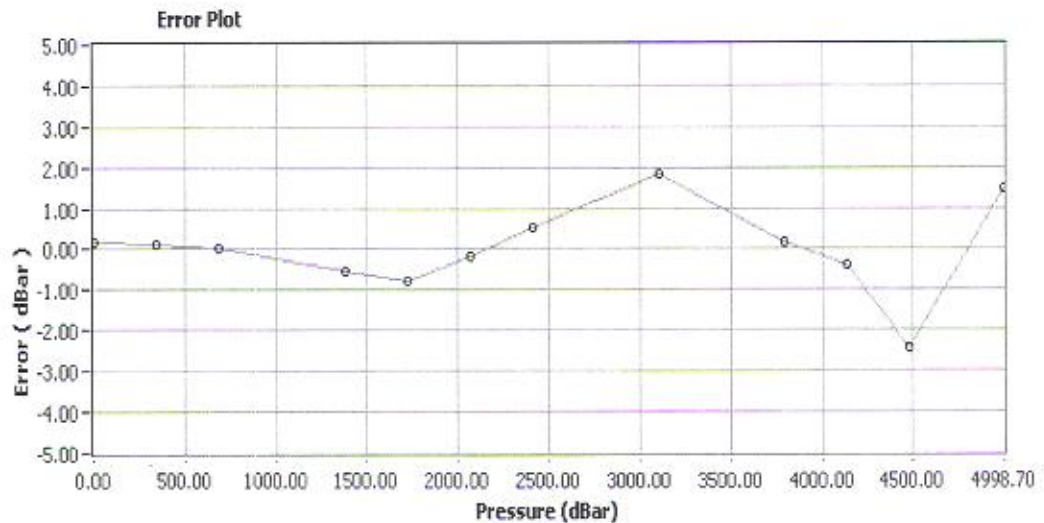

$$\text{dBar} = A + B \cdot \text{Raw} + C \cdot \text{Raw}^2 + D \cdot \text{Raw}^3$$

A=-7.966368E+3 G=
B=4.366591E-1 H=
C=-2.028614E-6 I=
D=2.866093E-11 J=
E= K=
F= L=

APPLIED Because it's not just 
MICROSYSTEMS

2071 Malaview Ave West, Sidney, British Columbia, Canada V8L 5X6
Phone: (250) 656-0771 Fax: (250) 655-3655
Canada & USA: 800-663-8721
Email: info@AppliedMicrosystems.com Web: <http://www.aml.bc.ca>