


Temperature Calibration

Date: 6/10/2008
Instrument SN: 004844
Calibrator: Les Woodland
RMS Error: 0.0325
Range: 0 to +45 Deg C

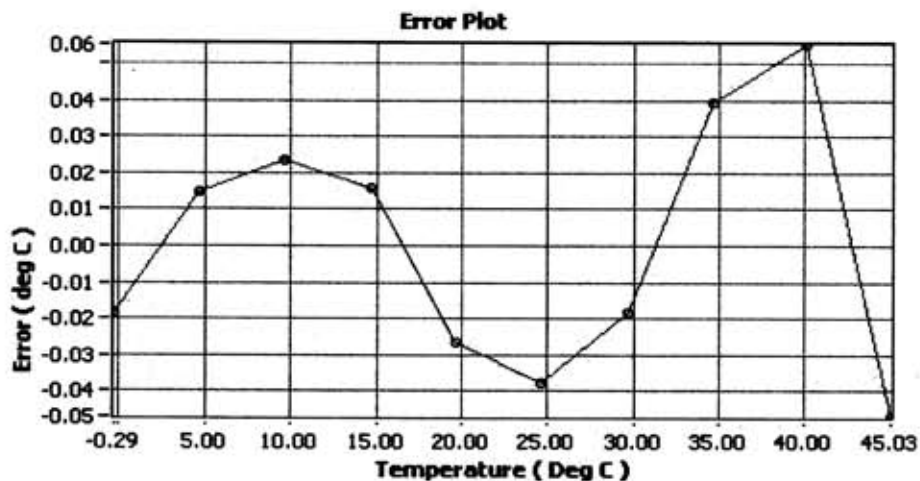

Deg C=A+B*Raw+C*Raw^2+D*Raw^3

Coefficients

A=-4.875283E+1

B=3.151186E-3

C=-5.518314E-8

D=5.633619E-13

APPLIED Because it's not just 
MICROSYSTEMS

2071 Malview Ave West, Sidney, British Columbia, Canada V8L 5X6
Phone: (250) 656-0771 Fax: (250) 655-3655
Canada & USA: 800-663-8721
Email: info@AppliedMicrosystems.com Web: <http://www.aml.bc.ca>